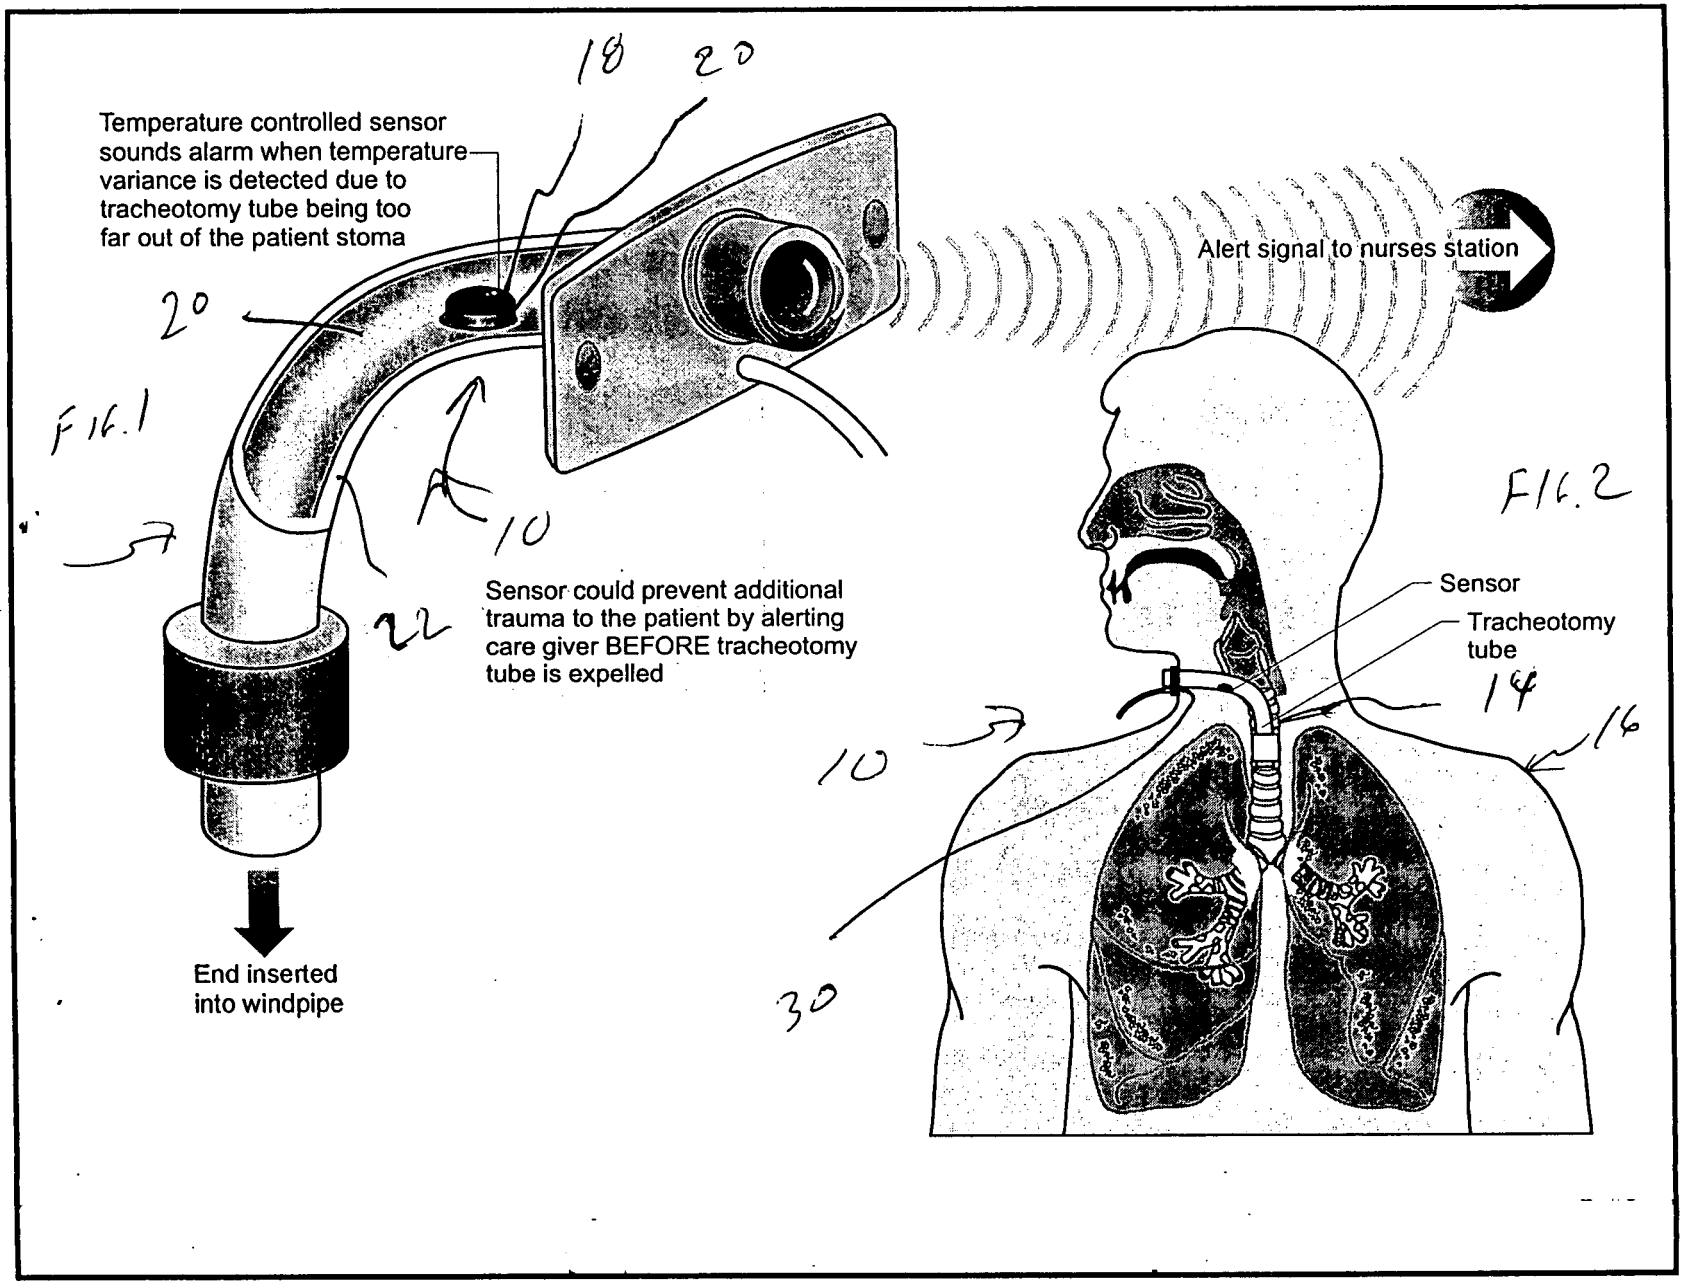
18
20
Temperature controlled sensor sounds alarm when temperature variance is detected due to tracheotomy tube being too far out of the patient stoma
20
Alert signal to nurses station
F16.1
10
12
22
Sensor could prevent additional trauma to the patient by alerting care giver BEFORE tracheotomy tube is expelled
End inserted into windpipe
F16.2
Sensor
Tracheotomy tube
14
16
10
30